MIDMARK®

Installation Instructions

9A258001 Pouch Rack For M4•9 Sterilizers

KIT COMPONENTS

Part Number	Description	Qty.
030-1163-00	Pouch Rack	2
• 003-1253-00	Installation Instructions	1

IMPORTANT INSTRUCTIONS

WARNING

Pouch Racks are for use *only* with pouched instruments. *Do not use for sterilization of dental handpieces.*

Only place tray with pouch racks on *bottom position* in chamber with *no* other trays in chamber.

INSTALLATION

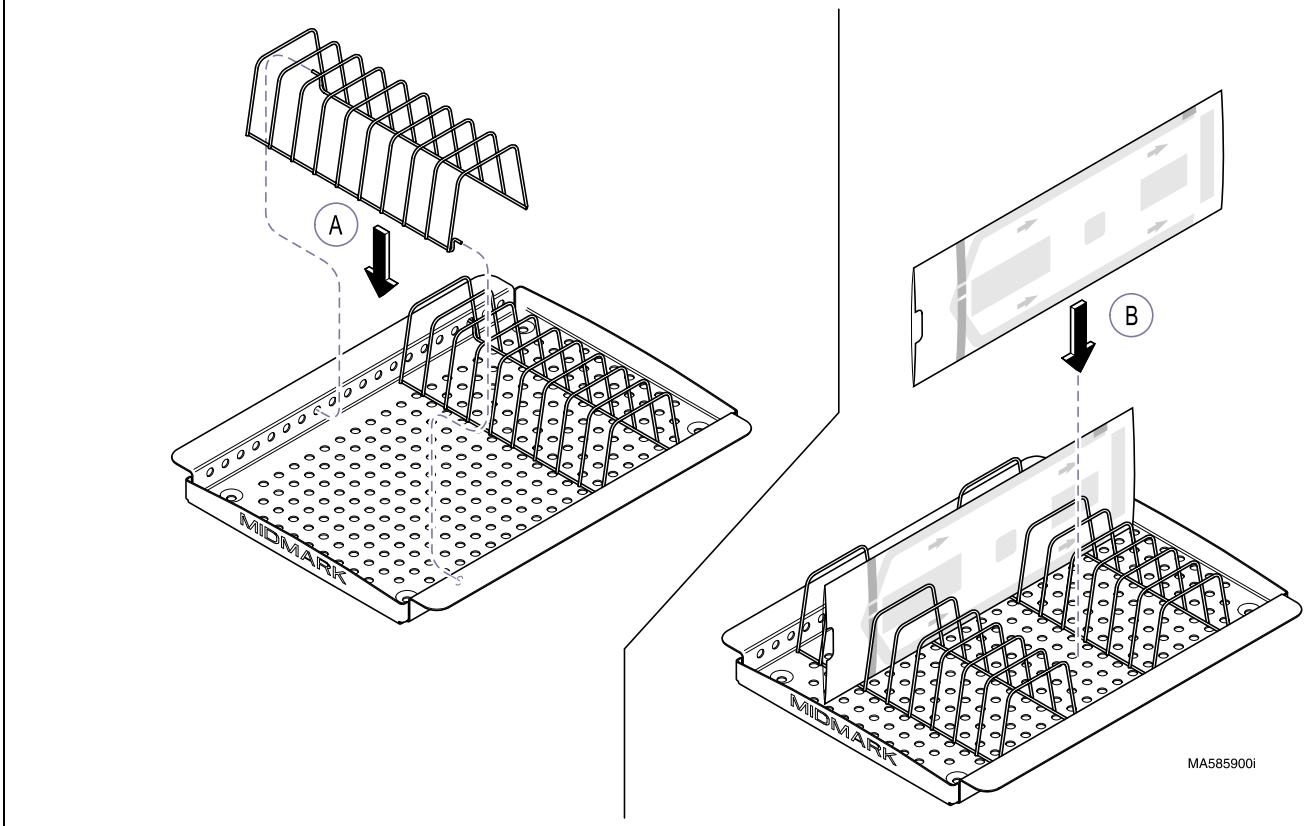

WARNING

Pouch Racks are for use *only* with pouched instruments.
Do not use for sterilization of dental handpieces.
Only place tray with pouch racks on *bottom position* in chamber with *no* other trays in chamber.

NOTE

One or two racks can be used on a tray. When using two racks, space racks evenly apart. Position pouched instruments in racks so when inserted into sterilizer the pouch(es) do not touch the chamber walls. Place tray containing pouch rack(s) in sterilizer chamber at the bottom position in tray rack. Do not place any other trays or cassettes above pouch racks.

A. Place the pouch racks into the tray as shown, inserting the wire tabs at each end of rack into holes of tray.

B. Position the pouched instruments evenly onto the racks and place assembly into sterilizer.

© Midmark Corporation - 2001

MIDMARK®
Midmark Corporation, Versailles, Ohio 45380 U.S.A.
(937) 526-3662 FAX (937) 526-5542

003-1253-00 Rev. A (8/01)